



Power Electronic Measurements

ROGOWSKI CURRENT
WAVEFORM TRANSDUCERS

INSTRUCTIONS FOR USE
RCTrms & RCTrms-3ph

POWER ELECTRONIC MEASUREMENTS Ltd.

Tel: +44 115 946 9657
Email: info@pemuk.com • Web: www.pemuk.com

INTRODUCTION 3

TECHNICAL SPECIFICATION 3

STANDARDS AND APPROVALS 4

OVERVIEW RCTRMS 5

OVERVIEW RCTRMS-3PH 6

SAFETY AND PRE-USE CHECKS 7

CONNECTIONS AND CABLING..... 9

SWITCHING ON 10

OBTAINING THE BEST MEASUREMENT 11

CLEANING AND DECONTAMINATION 12

WARRANTY..... 12

RETURNING YOUR RCT FOR RECALIBRATION OR REPAIR..... 12

INTRODUCTION

The RCTrms is a wide-bandwidth, flexible, clip-around current transducer for measuring ac currents.

PEM's Rogowski Current Waveform Transducers combine high bandwidth, safety, and the minimum disruption to the circuit under test. These instructions should be followed whenever the unit is used. They are intended to help you obtain the best and safest performance from the transducer.

Throughout this instruction sheet there are a number of warnings which must be observed to ensure safe operation of this unit. These warnings are identified by the following symbol:



The intended use is for the measurement of AC current. PEM accepts no responsibility for any damage resulting from careless use, or failure to observe these instructions.

TECHNICAL SPECIFICATION

Rated Current (Ip)	Refer to ID Label
Rated Output (Model Specific)	4 to 20mA (Full Scale) 0 to 5V (Full Scale)
Output Limit	150% FS
Output Load (Model Specific)	< 300Ω (4-20mA O/P) > 1kΩ (0-5V O/P)
Bandwidth (-3dB)	2Hz to 100kHz
Operating Temperature Range	-5°C to +65°C (<i>Integrator electronics</i>) -20°C to +80°C (<i>Coil and cable</i>)
Accuracy (typ.)	±1.5% of reading (10% to 150% FS, 25°C)
Absolute Max rms di/dt Ratings	0.24 kA/μs
Coil Insulation	2.0kV peak
Coil Bend Radius (Min.)	40mm


Supply Voltage		12Vdc (-10%) –to- 24Vdc (+20%)
Supply Power	RCTrms	0.7W (at rated output)
	RCTrms-3ph	2.1W (at rated output)
Supply Isolation		2.0kV dc
Environmental		Indoor use / Altitude up to 2000m
		Installation Category III, Pollution Degree 2.
		Max. Rel. Humidity: 80% up to 31°C Decreasing Linearly to 50% at 40°C

STANDARDS AND APPROVALS

EMC Approvals		EN61326-1:2013
		FCC Title 47 (CFR:2010, Part 15b)
Safety Approvals		EN61010-1:2010
		EN61010-2-032:2012
Quality System		ISO9001:2015




OVERVIEW RCTrms

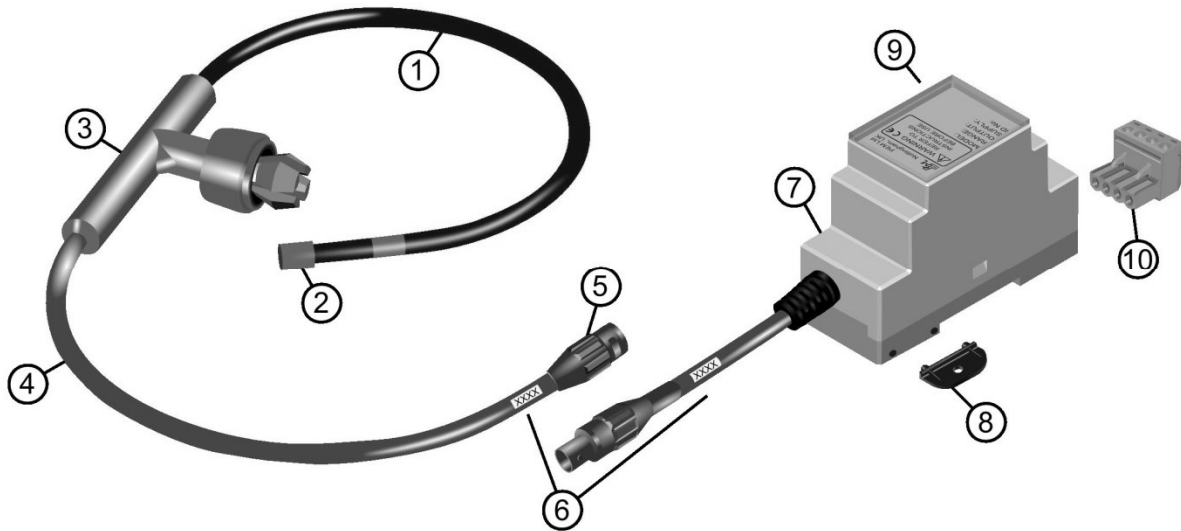

1. **Rogowski coil** (loop).
2. **'Free-end'** of the Rogowski coil
3. **Ferrule** (the connecting mechanism for closing the Rogowski coil).
4. **Cable connecting the Rogowski coil to the integrator** - doubly screened low noise co-axial cable.
 The Rogowski coil and connecting cable have double or re-enforced insulation.
5. **OPTION - BNC:BNC split in the cable** between the Rogowski coil and electronic integrator
6. **Coil / cable identification label on both BNC connector and enclosure**
7. **Plastic DIN rail mount electronic enclosure** housing the electronic integrator.
For mounting on DIN RAIL according to DIN EN 50 022
8. **Position for removable tabs to enable panel mounting of the enclosure.**
Mounting screw size is M4 (not supplied)
9. **Identification label** providing
 - Serial Number
 - Rated Primary Current (Ip)
 - Rated Output
 - Supply voltage
10. **Removable screw terminal connector plug for the SUPPLY and LOAD connections**

OVERVIEW RCTrms-3ph

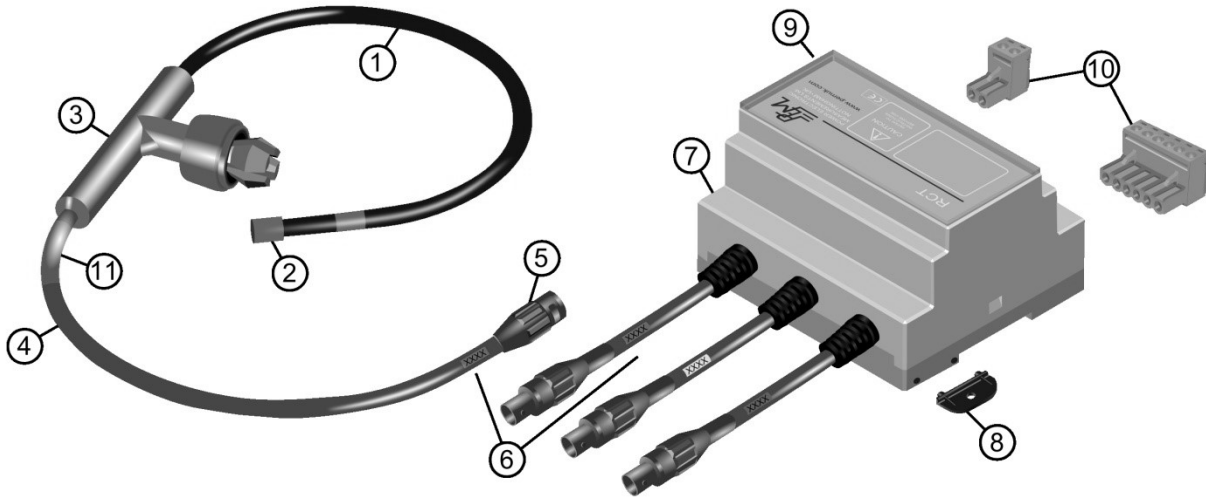

1. **Rogowski coil** (loop).
2. **'Free-end'** of the Rogowski coil
3. **Ferrule** (the connecting mechanism for closing the Rogowski coil).
4. **Cable connecting the Rogowski coil to the integrator** - doubly screened low noise co-axial cable.
 The Rogowski coil and connecting cable have double or re-enforced insulation.
5. **OPTION - BNC:BNC split** in the cable between the Rogowski coil and electronic integrator
6. **Coil / Cable identification label on both BNC connector and enclosure**
Colour coded serial numbers identify individual channels.
7. **Plastic DIN rail mount electronic enclosure** housing the electronic integrator.
For mounting on DIN RAIL according to DIN EN 50 022
8. **Position for removable tabs to enable panel mounting of the enclosure.**
Mounting screw size is M4 (not supplied)
9. **Identification label** providing
 - Serial Number
 - Rated Primary Current (Ip)
 - Rated Output
 - Supply Voltage
10. **Removable screw terminal connector plug for the SUPPLY and LOAD connections**

SAFETY AND PRE-USE CHECKS



The RCT does not provide protection of the user from electric shock whilst applying or removing the probe from HAZARDOUS LIVE conductors. Additional protective means are necessary to avoid electric shock from HAZARDOUS LIVE conductors which cannot be de-energised.

If HAZARDOUS LIVE voltages are present and accessible in the installation appropriate protective equipment must be used.

The Rogowski coil must not be used if the coil outer layer is damaged or in any way compromised.

The RCT must only be used in conjunction with properly earthed test equipment.

If the RCT is used in a manner not specified by the manufacturer the protection provided by the equipment may be impaired.

THE ROGOWSKI COIL



The integrity of the insulation around the Rogowski coil itself should be VISUALLY INSPECTED before use, and the unit must NOT BE USED if there are signs of damage.



When bending the flexible coil around a conductor, avoid tight bends and sharp edges that could damage the coil.



Do not bend the coil beyond the minimum bend radius.



The voltage rating (safe PEAK working voltage) is clearly labelled on the coil. The rating is 2kV peak. The removable silicone sleeve supplied with the coil provides additional mechanical protection only.

The rating is derived from the following standard test: All coils supplied by PEM including the ferrule connecting the coil to the cable are flash tested for 1 minute at 4kVrms using a 50Hz sinewave.



The user must ensure that the absolute maximum rated di/dt is not exceeded.




For permanent installation, the coil should be situated such that corona, which would eventually damage the coil insulation, cannot occur. For information regarding permanent installation of PEM's Rogowski coils on higher voltage equipment please consult PEM.




Voltage ratings are only valid if the 'free-end' of the coil is fully inserted into the socket, and remains fully inserted during use.

The 'free-end' will be fully inserted when the user feels the free-end of the coil engage with the internal click-in mechanism inside the ferrule.

Visual indication that the coil mechanism is fully inserted is provided by the black cable marker situated near the end of the coil, as shown on next page:

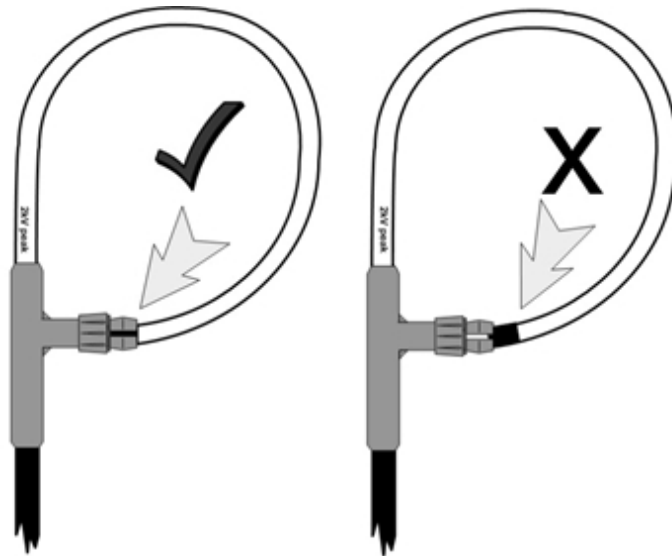

If the coil is to be left in-situ for any period of time or is used in an environment where the coil is subject to vibration the locking nut should be engaged as shown in the diagram below.

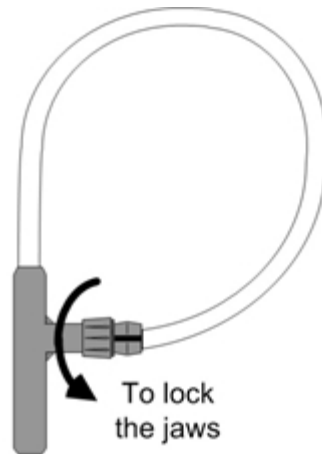

The locking mechanism must not be actuated at temperatures below 0°C

Care must be taken not to over-tighten the locking nut.

THE CABLE FROM COIL TO INTEGRATOR



The optional BNC:BNC cable split is manufactured with touch protected isolated BNC connectors. The two halves of the BNC cable split should be connected before the conductor under test (primary current) is energised.


THE INTEGRATOR




Terminal S2 should be connected to a LOAD which is connected to a safety earth.

CONNECTIONS AND CABLING

RCTrms

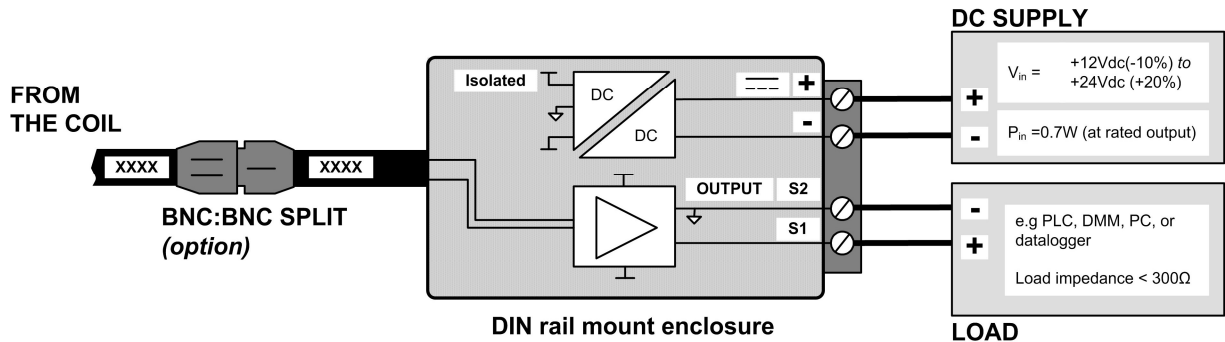

RCTrms-3ph

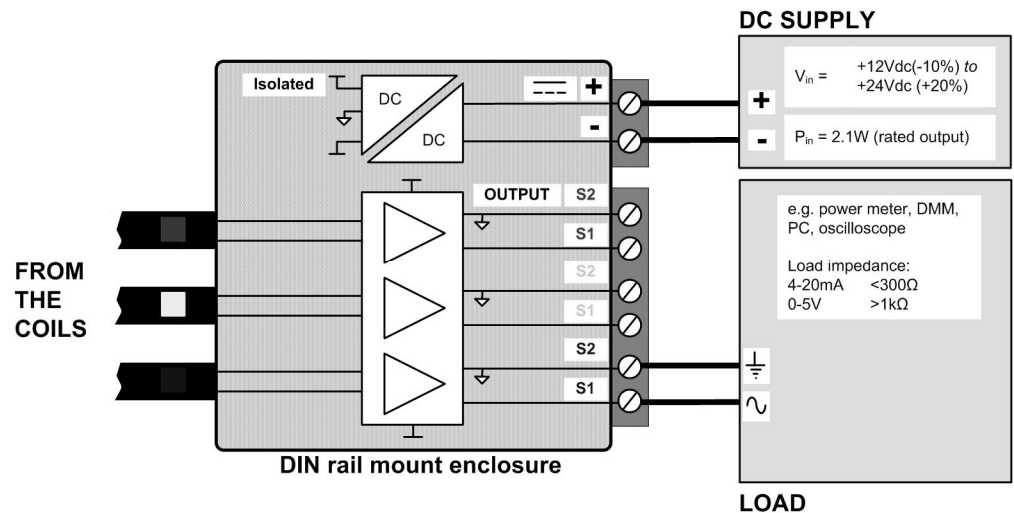

BNC:BNC SPLIT

Where the OPTIONAL BNC CONNECTOR is supplied check that the correct coil is connected to the integrator. The cable from both the coil and the integrator should have the same four or five digit ID label XXXX close to the BNC connection.

The integrator is calibrated for a given coil and the correct coil must be used to ensure rated accuracy. The coils and integrator must not be swapped.

DC SUPPLY

Explanation of symbols identifying the SUPPLY connections

- Direct current
- $+/-$ Positive / Negative terminal

The user must power the RCT with a suitable external DC power supply which should have the CE mark if the customer requires this certification.

The cable connecting the RCT to the DC supply should be dual-core or twisted pair power cable of sufficient rating. The power supply cable should be connected to the rising clamp screw terminals:

Max / Min wire size: 4.0 mm² / 0.5 mm²

Rated torque / screw size: 0.5 Nm / M3

In some electrically noisy environments it is best practice to use a shielded twin core power cable. In such cases the shield should be connected to the ground of the external dc power supply and left open circuit at the end connected to the RCTrms.

LOAD

Explanation of symbols identifying the LOAD connections

- (S1) Output signal
- (S2) Output signal

The cable connecting the RCT to the LOAD should be dual-core or twisted pair power cable of less than 5m and of sufficient rating. The load cable should be connected to the rising clamp screw terminals:

Max / Min wire size: 4.0 mm² / 0.5 mm²

Rated torque / screw size: 0.5 Nm / M3

In some electrically noisy environments it is best practice to use a shielded or doubly shielded cable. In such cases the outer shield should be connected to the ground of the load measuring device and left open circuit at the end connected to the RCT.

SWITCHING ON

Mount the electronic enclosure housing the electronic integrator on a suitable DIN rail. Alternatively fit the two removable panel mount tabs to the enclosure and mount to a suitable panel. In both cases ensure that there is access to the removable PCB mount terminal block.



Before switching on the RCT and taking a measurement refer to SAFETY AND PRE-USE CHECKS and CONNECTIONS AND CABLING to ensure safe operation.



The user is advised to de-energise the circuit under test first. If the probe is being fitted to a live circuit the user must ensure the use of appropriate personal protective equipment.

The transducer is switched ON by supplying the correct DC SUPPLY to the RCT. The DC supply voltage is clearly shown on the identification label on the electronic enclosure and is fully specified in TECHNICAL SPECIFICATION' of this manual.


After switch-on the RCT requires a settling time to attain its quiescent state before providing correct current measurement. The time, which depends on warm-up and low frequency bandwidth, can be as long as 2 minutes.

Having carried out the visual inspection of the Rogowski coil, un-clip the coil and wrap around the de-energised conductor under test, fully inserting the free-end of the Rogowski coil into the ferrule as shown in SAFETY AND PRE-USE CHECKS.

The user is now ready to re-energise the conductor under test and take measurements.

OBTAINING THE BEST MEASUREMENT

The Rogowski coil should be positioned so that the conductor under test is encircled by the coil but is not adjacent to the cable attachment (see picture below). The RCTrms has been calibrated with the conductor near the centre, and this is the ideal position.

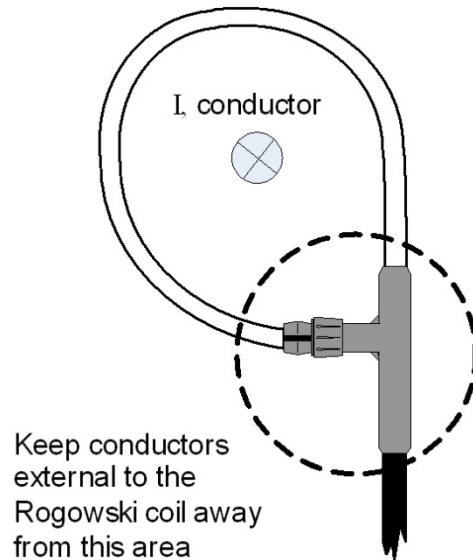

The sensitivity of the RCTrms to currents that do not pass through the coil is very small, provided that such currents are no greater than the RCTrms rating or such currents are relatively distant from the coil. In the vicinity of a multi-turn inductor the 'H' field is far stronger than from a single conductor carrying the same current, and such positions should be avoided.

Similarly if there is a surface with a high voltage very close to the coil, and the voltage is subject to high rates of change (e.g. several 100 V/ μ s) or high frequency oscillations in the MHz range, then measurement error can arise due to capacitive coupling to the coil.

As a check on any unwanted response to adjacent fields, it is wise to display the output of the RCTrms when close to (but not encircling) the conductor whose current is to be measured. This will reveal the magnitude of any unwanted response to currents close to but outside the coil.

CLEANING AND DECONTAMINATION

To prevent surface contamination the Rogowski coil and cable should be inspected regularly.

To clean the coil and cable, first disconnect from the power source and any external circuits, then use a mild detergent and damp cloth to remove any contamination and dry thoroughly with a clean cloth before placing back in to service.

WARRANTY

The coil is guaranteed to be free from defects due to materials and workmanship for 12 months and the integrator for 24 months from the date of despatch from Power Electronic Measurements Ltd.

In the event of a defect where the transducer has not been misused the RCT should be returned to PEM with all freight charges to be paid by the customer. Correction shall be in the form of repair or replacement.

RETURNING YOUR RCT FOR RECALIBRATION OR REPAIR

To return the RCT to PEM for recalibration or repair please contact PEM in advance for shipping instructions (refer to our website for contact details and our returns procedure).

For technical updates or enquiries and the latest product releases please consult

www.pemuk.com

POWER ELECTRONIC MEASUREMENTS Ltd.

Gloucester House, Wellington Street, Long Eaton, Nottingham, NG10 4HS, U.K.

Tel: +44 115 946 9657

Email: info@pemuk.com